

Arrhythmia Detection based on Morphological and Time-frequency Features of T-wave in Electrocardiogram

Elham Zeraatkar, Saeed Kermani, Alireza Mehridehnavi¹, A. Aminzadeh², E. Zeraatkar³, Hamid Sanei⁴

Departments of Physics & Biomedical Engineering and ⁴Internal Medicine, ¹Medical Image & Signal Processing Research Center, Isfahan University of Medical Sciences, Isfahan, ²Navigation and Control, Marine Industries Organization, ³Electronic and Computer Engineering, Shiraz University, Shiraz, Iran

ABSTRACT

As the T-wave section in electrocardiogram (ECG) illustrates the repolarization phase of heart activity, the information which is accumulated in this section is so significant that it can explain the proper operation of electrical activities in heart. Long QT syndrome (LQT) and T-Wave Alternans (TWA) have imperceptible effects on time and amplitude of T-wave interval. Therefore, T-wave shapes of these diseases are similar to normal beats. Consequently, several T-wave features can be used to classify LQT and TWA diseases from normal ECGs. Totally, 22 features including 17 morphological and 5 wavelet features have been extracted from T-wave to show the ability of this section to recognize the normal and abnormal records. This recognition can be implemented by pre-processing, T-wave feature extraction and artificial neural network (ANN) classifier using Multi Layer Perceptron (MLP). The ECG signals obtained from 142 patients (40 normal, 47 LQT and 55 TWA) are processed and classified from MIT-BIH database. The specificity factor for normal, LQT, and TWA classifications are 99.89%, 99.90%, and 99.43%, respectively. T-wave features are one of the most important descriptors for LQT syndrome, Normal and TWA of ECG classification. The morphological features of T-wave have also more effect on the classification performance in LQT, TWA and normal samples compared with the wavelet features.

Key words: ECG, feature extraction, morphology, neural network, T-wave, wavelet

INTRODUCTION

The long QT syndrome (LQTS), T-wave alternans (TWA), and ventricular tachyarrhythmia (VT) are some of the common cardiac diseases which cause sudden cardiac death (SCD) in the world.^[1,2] Many studies have been developed to detect an abnormal sinus ECG based on the features of ECG signal. Most of these articles use QRS complex to indentify the arrhythmia of the heart. One of the traditional methods has been performed by Jain^[3] that digitized and represented each ECG lead by its z-domain modes to enhance the discrimination of the subtle changes in P, QRS, and T sections, the derivatives of the waves are employed for extraction of the modes. Lin *et al.*^[4] used linear prediction to extract features from QRS complexes. Osowski *et al.*^[5] applied fuzzy neural network to ECG beat recognition and classification and the features drawn from the higher order statistics have been proposed in the study. Also Engin^[6] performed similar method and used autoregressive model coefficients, higher-order cumulant, and wavelet transform variances as features to enhance the performance. Jekova *et al.*^[7] implemented four different classifiers based on 26 morphological features

which have been extracted from lead I, II, and the Frank Leads or vector cardiograph (VCG) trajectory signals, such as area, slopes, peaks, time intervals, and VCG diagram in QRS complex. Asl *et al.*^[8] presented an effective cardiac arrhythmia classification algorithm based on the generalized discriminant analysis (GDA) to reduce feature scheme using support vector machine (SVM) classifier. Initially, 15 different linear and nonlinear features have been extracted from QRS complex and then reduced to only 5 features by the GDA technique. Vaglio *et al.*^[9] and Couderc *et al.*^[10] implemented a computer algorithm to identify the differentiation of LQT1 and LQT2 carriers' base on T-wave morphology features, such as the Q to T-peak (QT-peak), the T-peak to T-end interval, T-wave magnitude, and T-loop slopes in these studies.

In recent works,^[11,12] simulated and synthetic TWA signals were generated. These augmented beats were detected using wavelets and 91% sensitivity was achieved. In other studies, wavelet/FFT^[13] and correlation/FFT methods^[14] were also considered.

The novelty of this work can be explained as follows. In

Address for correspondence:

Dr. Saeed Kermani, Department of Physics and Biomedical Engineering, Isfahan University of Medical Sciences and Health Services(IUMS), Hezar Jarib Street, Isfahan , Iran. E-mail: kermani@med.mui.ac.ir

this study, diseases are recognized from the beats that seem normal (sinus ECG), but in fact, they belong to LQT or TWA classes. However, other works only classify heartbeat types.^[11-14] Consequently, previous studies are not comparable with this approach.

In this article, diseases are classified by the following procedures: Pre-processing, QRS-complex detection, T-wave detection, features extraction from T-wave section (morphological and wavelet coefficients), and classification using MLP artificial neural networks.

METHOD

Arrhythmia detection algorithm is implemented as follows: (a) recalling suitable ECG database; (b) pre-processing; (c) QRS-complex detection; T-wave detection; (d) feature extraction from T-wave; and (e) MLP classifier as shown in Figure 1.

ECG Database and Pre-processing

In this article, the MIT/BIH database^[15-17] has been chosen with 40 normal records, 47 LQT syndrome records, and 55 sets of TWA arrhythmia from 142 ECG recordings Lead I with 128Hz, 250Hz, and 500Hz sampling rate, respectively.

Before applying detections, feature extraction and classifying procedure in this experiment, several pre-processings are necessary to obtain an appropriate result and reduce errors in processing and detection phases. Most common artifacts and drifts appear by 50 Hz of 60 Hz power line interface, muscle contractions of electromyography noise (EMG), baseline drift and ECG amplitude modulation with respiration, and ECG corruption with abrupt baseline shift.^[18] To avoid these disturbances, the following filters are applied:

- To eliminate power line effect a notch filter^[19] has been developed with the following transfer function:

$$H(z) = \frac{(z - z_1)(z - z_2)}{(z - p_1)(z - p_2)} \quad (1)$$

Where

$$z_1 = \cos(\omega_0) + j \sin(\omega_0) \quad (2)$$

And

$$z_2 = \cos(\omega_0) - j \sin(\omega_0) \quad (3)$$

are the zeros of transfer function and

$$p_1 = k[\cos(\omega_0) + j \sin(\omega_0)] \quad (4)$$

And

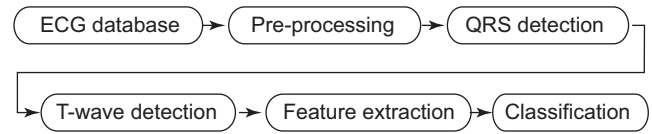


Figure 1: Block diagram of algorithm

$$p_2 = k[\cos(\omega_0) - j \sin(\omega_0)] \quad (5)$$

are the poles of the transfer function with pole/zero ratio $k=0.9$, cutoff frequency $\omega_0 = \pm [f_0 / f_s] \times (2\pi r)$, center frequency $f_0 = 50$ Hz and sampling rate f_s .

- To reduce the effect of EMG noise, a discrete Butterworth filter with order 8 and cutoff frequency $f_c = 70$ Hz and sampling rate f_s .
- For decreasing the amount of ECG baseline drift with respiration the following method is applied:^[20]
 - Computing median of the ECG
 - Shifting ECG by this median value
 - Fitting a 4th degree polynomial to the shifted ECG
 - Shifting ECG by this calculated polynomial
 - Detecting the R peaks of ECG
 - Computing median of each RR interval the ECG
 - Shifting each RR interval by its median value
- For ECG corruption with abrupt baseline shift the algorithm mentioned in part(c) is also applied to the ECG signal.

Noise reduction and robustness of implemented algorithm with above artifacts have been discussed in another study.^[21]

QRS Complex Detection

In this section, the QRS complexes of the ECG are detected and eliminated from overall ECG to prepare the signal for T-wave detection. This will be implemented by the following steps:^[22]

- Recall ECG signal $S(n)$ and compute square of this signal after pre-processing:

$$TS1(n) = S(n) * S(n) \quad (6)$$

- Evaluate the steepest windowed gradient of $TS1(n)$ by using a rectangular sliding window with 11 points from sample $n-5$ to $n+5$:

$$G1(n) = TS1_{\max}(w) - TS1_{\min}(w) \quad (7)$$

- Smooth the signal by using a moving average method from sample $n-5$ to $n+5$ with center n :

$$FG1(n) = \frac{1}{11} \sum_{i=n-5}^{n+5} G1(i) \quad (8)$$

4. Normalize the following values by their respective maximum peak amplitude: $S(n)$, $TS1(n)$, $G1(n)$ and $FG1(n)$.

5. Transform the ECG signal by a sigmoid function:

$$TS2(n) = 1 - \frac{2}{e^{2S(n)} + 1} \quad (9)$$

6. Evaluate the steepest windowed gradient of $TS2(n)$ by using a rectangular sliding window with 11 points from sample $n-5$ to $n+5$.

$$G2(n) = TS2_{\max}(w) - TS2_{\min}(w) \quad (10)$$

and smooth it to $FG2(n)$ like step 3.

7. Normalize the following values by their respective maximum peak amplitude: $TS2(n)$, $G2(n)$ and $FG2(n)$.

8. Multiply by ECG with $FG2(n)$:

$$TS3(n) = FG2(n) * S(n) \quad (11)$$

9. Evaluate the steepest windowed gradient of $TS3(n)$ by using a rectangular sliding window with 11 points from sample $n-5$ to $n+5$.

$$G3(n) = TS3_{\max}(w) - TS3_{\min}(w) \quad (12)$$

and smooth it to $FG3(n)$.

10. Normalize the following values by their respective maximum peak amplitude: $TS3(n)$, $G3(n)$ and $FG3(n)$.

11. Compute:

$$TS4(n) = FG1(n) + FG3(n) \quad (13)$$

12. Shift the resulting signal by median 'm':

$$TS4m(n) = TS4(n) - m \quad (14)$$

13. Normalize $TS4m(n)$ as:

$$Pre_F_Q(n) = TS4m(n) / \max(\text{abs}(TS4m(n))) \quad (15)$$

14. $F_Q(n)$ is derived by retaining the amplitude values of Pre_F_Q exceeding 5% of its maximum peak amplitude and reducing the remaining to zero:

$$F_Q(n) = \begin{cases} Pre_F_Q(n) & \text{if } Pre_F_Q(n) > 0.05 \\ 0 & \text{otherwise} \end{cases} \quad (16)$$

15. C_Q is the proposed feature signal employed for identifying QRS out of ECG signal. This signal is digitalized version of $F_Q(n)$:

$$C_Q(n) = \begin{cases} 1, & \text{if } F_Q(n) > 0.05 \\ 0, & \text{otherwise} \end{cases} \quad (17)$$

T-Wave Detection

To extract features from T-wave section of ECG signal the interval of T-wave segments should be separated from other parts of signal. There are several methods to detect this section.^[23-26] One of the latest approaches can be done by the following steps after eliminating negative values and QRS parts of ECG signal in each of the following steps:

1. $fc1$: Feature #1 is calculated from the first derivative of ECG signal
2. $fc2$: Feature #2 is calculated from filtered gradient, which means the ECG signal passes through a sigmoid function, windowed gradient, and smoothed by a moving average window
3. $fc3$: Feature #3 is calculated from the product of filtered gradient ECG and $fc2$
4. $fc4$: Feature #4 is calculated from the combination of $fc1$, $fc2$, $fc3$ and absolute value of ECG: $|fc1 + fc2 + fc3 + |S(n)| * |S(n)|$
5. $fc5$: Feature #5 is calculated from another combination of $fc1$, $fc2$, $fc3$ and absolute value of ECG: $|fc1 + fc2 + fc3 + |S(n)|$.

Then the summation of these five features is computed by the following formula:

$$Pre_F_{NQ}(n) = fc1(n) + fc2(n) + fc3(n) + fc4(n) + fc5(n) \quad (18)$$

Finally the main feature will be computed by:

$$F_{NQ}(n) = \begin{cases} Pre_F_{NQ}(n), & \text{if } 0 \leq Pre_F_{NQ}(n) \leq 1 \\ 1, & \text{if } Pre_F_{NQ}(n) > 1 \\ 0, & \text{if } Pre_F_{NQ}(n) < 1 \end{cases} \quad (19)$$

The values greater than 2% of the maximum of this feature will show the P-wave and T-wave regions in ECG which is marked as pulses. The pulses occur before QRS complexes indicate P-waves and the pulses after QRS shows T-waves as depicted in Figure 2. The details and exact formulation of this procedure can be found in articles.^[27]

Feature Extraction

Detecting T-waves from ECG signal prepares the field to extract necessary descriptors from these parts of signal. Totally, 22 features have been considered and extracted from T-wave which consist of two fundamental types of features; There are 17 morphological features and 5 wavelet features. Morphological features include amplitude of T-wave, static and dynamic rising and falling slopes, areas of rising and falling segments, five slopes and five areas respect to split

falling segment of T-wave into five sections. The other type of features is variances of Daubechies wavelet coefficients which decomposed T-wave segment into five levels. These features have been summarized in Table 1 and shown in Figure 3a-d. As it is evident in Figure 4, the T-wave of three

classes (normal, LQT, and TWA) are very similar together and cannot recognize simply. For this reason, 22 features are selected to classify these types from each other.

Classification

The classification of diseases is based on Multi Layer Perceptron (MLP) using Artificial Neural Network (ANN)^[28,29] with 22 neurons at input, 14 at hidden layer, and one at output which generates 3 integer numbers for 3 classes. All

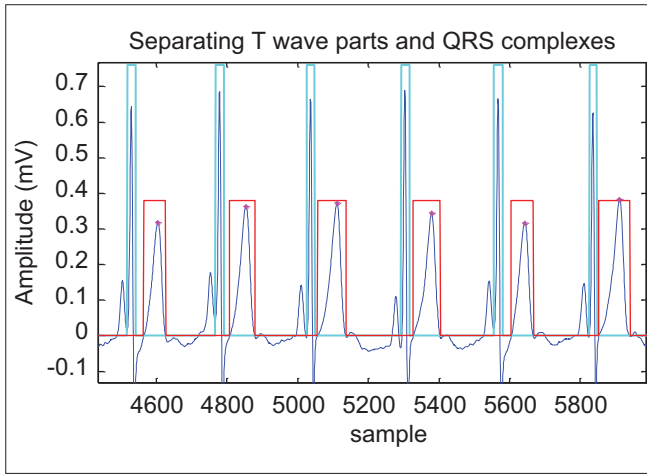


Figure 2: QRS-Complex and T-Wave separating pulses

Table 1. Feature description extracted from T-wave

Feature No.	Notation	Description
1	m_{sr}	Static rising slope
2	m_{sf}	Static falling slope
3	m_{dr}	Dynamic rising slope
4	m_{df}	Dynamic falling slope
5	T_p	Maximum peak of T-wave
6	A_r	Rising segment Area
7	A_f	Falling segment Area
8-12	A_{f1}, \dots, A_{f5}	Falling segment area split into five parts
13-17	m_{f1}, \dots, m_{f5}	Falling segment slopes split into five parts
18-22	$\sigma_{w1}, \dots, \sigma_{w5}$	Variance of wavelet coefficients

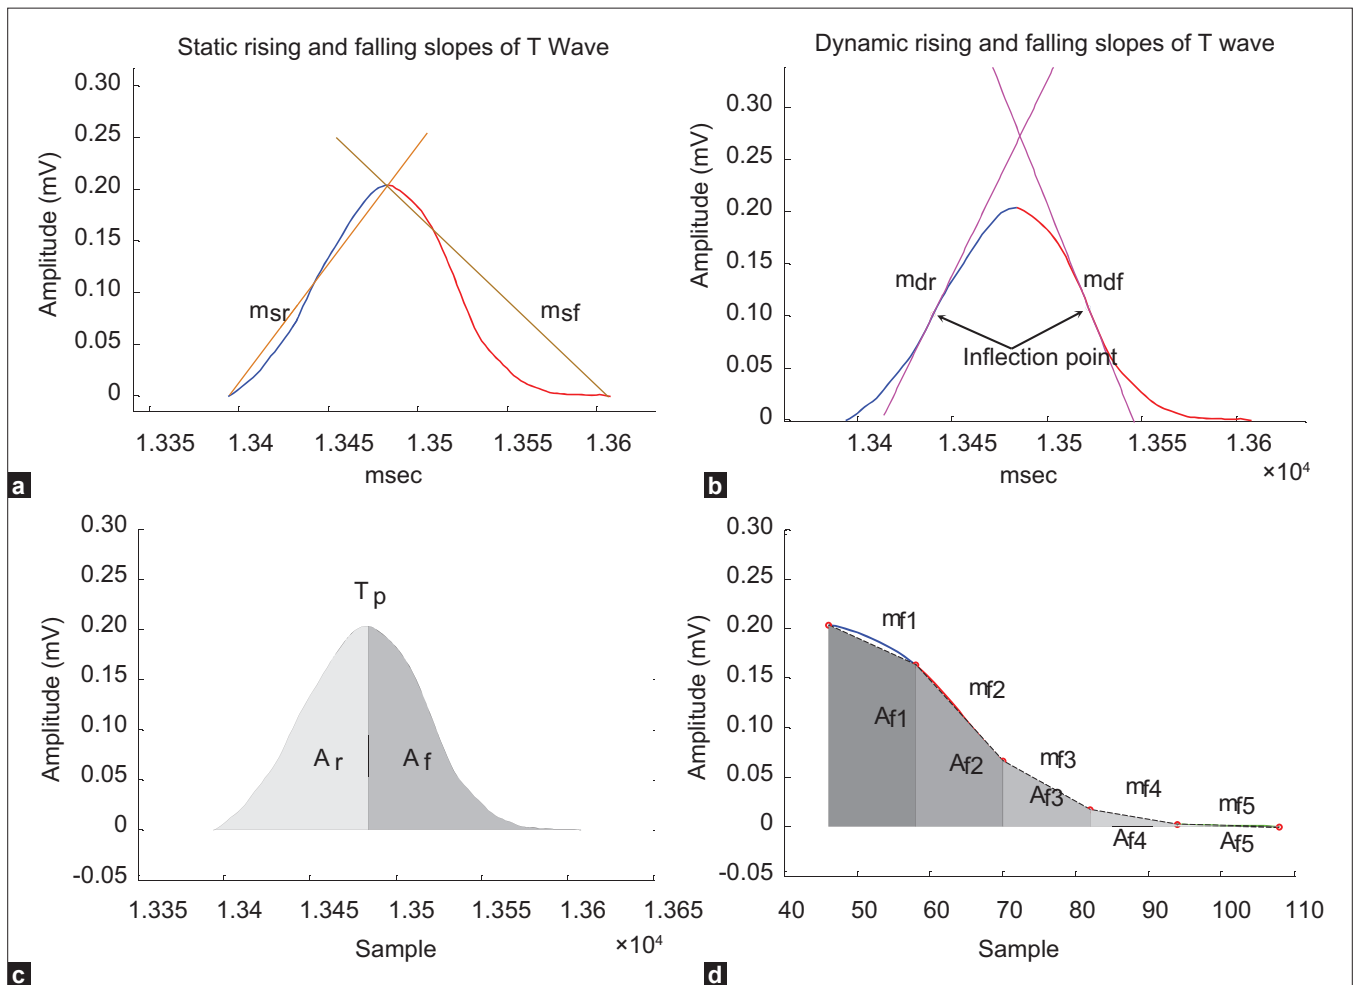


Figure 3: Some morphological features extracted from T-Wave. (a) Dynamic slopes and inflection points of T-wave; (b) Static slopes of T-wave; (c) Rising and falling areas of T-wave; (d) Falling area and slopes of T-wave separating to segments

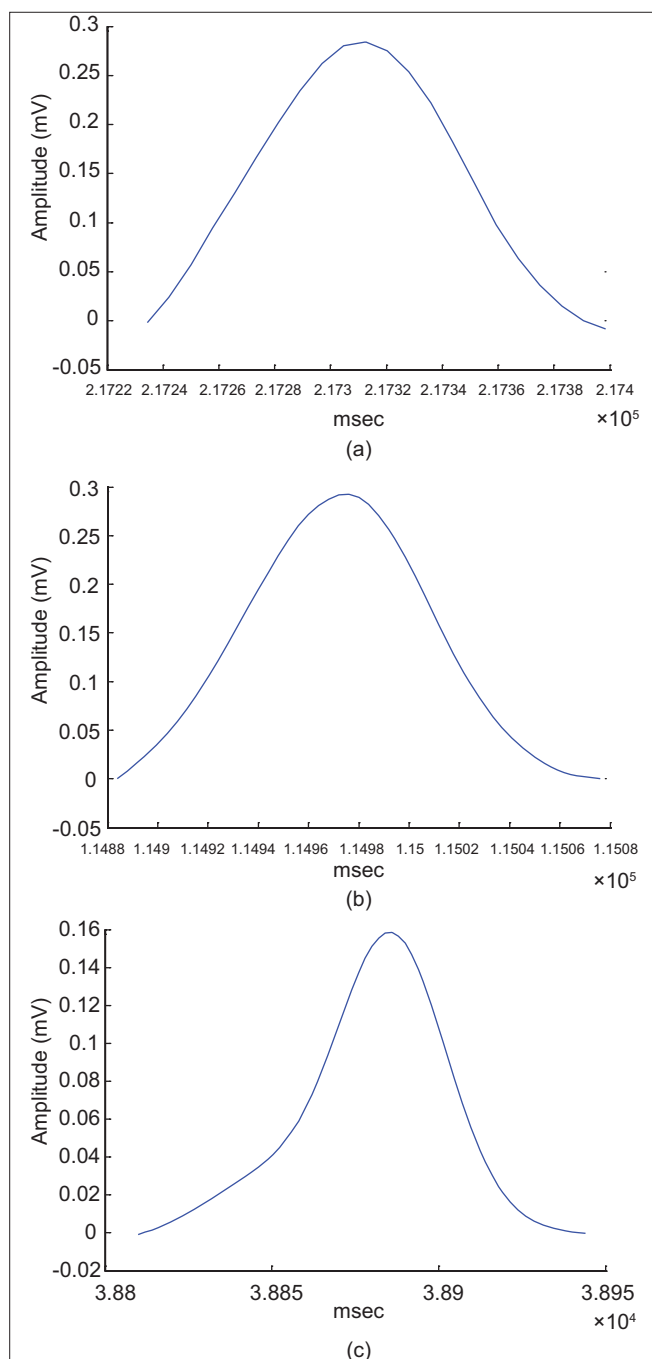


Figure 4: Typical wave forms from T-wave section of (a) Normal (b) LQT and (c) TWA

of the 22 features have been scaled and applied to the input of ANN are used and implemented to an appropriate ANN architecture for training and testing as shown in Figure 5. The output of network is determined as normal, LQT, and TWA abnormalities.

RESULTS

The discussed approach is simulated and applied to normal and abnormal TWA and LQT databases of MIT/BIH arrhythmia

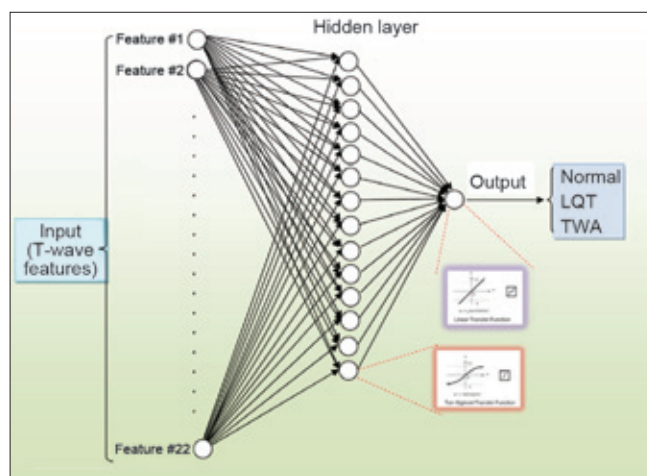


Figure 5: MLP neural network architecture

recordings. The input vectors, which are developed from T-wave features of ECG, are collected and separated into two parts for training and testing the MLP neural network. There are 22 scaled and extracted features containing 17 morphological and 5 wavelet features. Since the T-wave part of an ECG, specially falling interval, illustrates the repolarization phase of heart activity, the information which is accumulated in this section is so significant that it can explain the proper operation of electrical activities in heart. Therefore, these features are rich descriptors for heart performance.

The MIT-BIH database^[15-17] has been chosen for implementation of the algorithm in this study. The samples have been taken from three ECG types totally 142 records with the following properties:

- MIT-BIH Normal Sinus Rhythm Database (40 records, 128Hz sampling rate);
- The QT Database (47 records, 250Hz sampling rate);
- T-Wave Alternans Challenge Database (55 records, 500Hz sampling rate).

The learning process to train MLP neural network has been implemented with three different learning sets: 50, 60, and 70% heartbeats of total recordings. For estimating the performance of discussed approach, three different feature vectors have been developed and tested: Only wavelet features, only morphological features, and both features together. Finally, four performance indices based on ROC (Receiver Operating Characteristics) were computed for normal and abnormal classes: sensitivity (Se_i), specificity (Sp_i), positive predictive value (PPV_i) and negative predictive value (NPV_i). They are calculated according to the following relations:^[30]

$$Sp_i = \frac{TN_i}{TN_i + FP_i}, \quad Se_i = \frac{TP_i}{TP_i + FN_i} \quad (20)$$

$$NPV_i = \frac{TN_i}{TN_i + FN_i}, \quad PPV_i = \frac{TP_i}{TP_i + FP_i}$$

where TP_i are the number of true positives, TN_i are true negatives, FP_i are false positives, and FN_i are false negatives. The results are representation listed in Tables 2-4 according to different learning sets and descriptor vectors. As it is evident in the results, the network performance differs by changing learning sets and changing the types of features.

The statistical measurements for three features have been depicted in Figure 6 to show the ability of features for the classification of diseases. This describes that the morphological properties, such as falling area and falling slope of T-wave, have different distribution, mean, and variance and can be used for ECG classification.

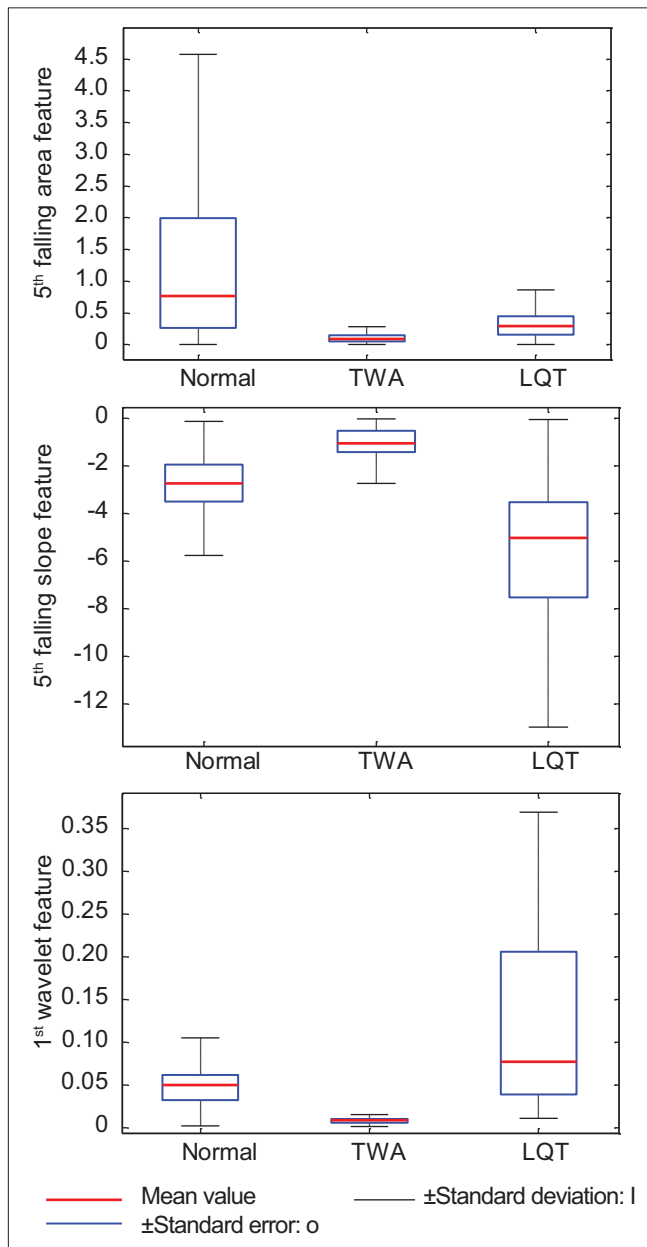


Figure 6: Statistical distribution for three features: 5th falling area, 5th falling slope and 1st wavelet coef

CONCLUSIONS

In previous biomedical studies, detecting normal and abnormal beats are considered by applying several methods. These procedures verify the variations of one

Table 2: Testing results for normal ECG signal

Normal	Feature set #1 5 descriptors (Wavelets)	Feature set #2 17 descriptors (Morphology)	Feature set #3 22 descriptors (Total)
Learning set #1 (50% of data)			
Index			
Sp†	95.01	99.43	99.8
Se‡	90.45	98.64	99.12
NPV§	91.61	98.77	99.20
PPV*	94.29	99.37	99.78
Learning set #2 (60% of data)			
Index			
Sp	96.52	99.77	99.79
Se	90.54	98.34	99.18
NPV	91.80	98.51	99.25
PPV	95.96	99.74	99.78
Learning set #3 (70% of data)			
Index			
Sp	96.77	99.66	99.89
Se	88.50	98.97	99.09
NPV	90.16	99.06	99.17
PPV	96.18	99.63	99.88

† Sp – Specificity; ‡ Se – Sensitivity; § NPV – Negative predictive value;
* PPV – Positive predictive value; Figures are in percentage

Table 3: Testing results for LQT ECG signal

LQT	Feature set #1 5 descriptors (Wavelets)	Feature set #2 17 descriptors (Morphology)	Feature set #3 22 descriptors (Total)
Learning set #1 (50% of data)			
Index			
Sp	95.82	99.40	99.89
Se	73.07	96.51	98.45
NPV	88.74	98.44	99.30
PPV	88.78	98.65	99.76
Learning set #2 (60% of data)			
Index			
Sp	93.93	99.46	99.90
Se	70.47	96.35	99.24
NPV	87.55	98.36	99.65
PPV	84.02	98.78	99.78
Learning set #3 (70% of data)			
Index			
Sp	95.25	99.32	99.89
Se	71.77	98.75	99.71
NPV	88.10	99.43	99.96
PPV	87.33	98.52	99.76

† Sp – Specificity; ‡ Se – Sensitivity; § NPV – Negative predictive value;
* PPV – Positive predictive value; Figures are in percentage

Table 4: Testing results for TWA ECG signal

TWA	Feature set #1 5 descriptors (Wavelets)	Feature set #2 17 descriptors (Morphology)	Feature set #3 22 descriptors (Total)
Learning set #1 (50% of data)			
Index			
Sp	86.95	97.98	98.96
Se	86.64	97.34	99.56
NPV	96.02	99.27	96.27
PPV	64.13	92.87	99.88
Learning set #2 (60% of data)			
Index			
Sp	85.15	97.72	99.25
Se	81.11	98.30	99.37
NPV	94.38	99.53	99.83
PPV	59.44	92.05	97.25
Learning set #3 (70% of data)			
Index			
Sp	84.10	99.03	99.43
Se	84.69	97.49	99.73
NPV	95.43	99.33	99.93
PPV	58.34	96.35	97.84

† Sp – Specificity; ‡ Se – Sensitivity; § NPV – Negative predictive value;

* PPV – Positive predictive value; Figures are in percentage

beat against others to find out abnormal beats. Regarding the new suggestions of cardiologists, some diseases, such as LQT and TWA, have imperceptible effect on time and amplitude of T-wave interval. In contrary to previous articles, in this work, disease detection (LQT syndrome and TWA) has been performed using apparently normal beats.

In some researches, several algorithms have been developed for T-wave detection. The accuracy reported in these articles is satisfactory.^[24-26,28,29,31] In this study, the T-wave detection based on threshold method developed in^[28] with 96.98% accuracy is used. This performance is more accurate compared with other methods.

According to the achieved results, it is obvious that T-wave features in sinus ECG signals have the capability to separate these diseases. Since the falling slope of the T-wave is associated with the repolarization phase of heart activity and preparing of heart muscles for next oscillation, this section contains significant morphological descriptors and has the necessary information to classify heartbeats. The specificity of mentioned approach depends on the quantity of learning set and feature types for neural network training. The morphological features of T-wave have also more effect on the classification performance in LQT, TWA, and normal samples compared with wavelet features.

ACKNOWLEDGMENT

This study was supported by Isfahan University of Medical Sciences

and Shiraz Kowsar Heart Clinic, with special thanks to Dr. M.H. Nikoo, Dr. P. Setoodeh, Ms. N. Karami and Mr. A. Fakhrpour.

REFERENCES

1. Takagi M, Yoshikawa JT. Wave alternans and ventricular tachyarrhythmia risk stratification: A Review. *Indian Pacing Electrophysiol J* 2003;3: 67-73.
2. Bernardo D, Murray A. Explaining the T-wave shape in the ECG. *Nature* 2000;403:40.
3. Jain VK. ECG waveform feature extraction and its application to automated prognosis. *Int J Parallel Programming* 1973;2:231-47.
4. Lin KP, Chang WH. QRS Feature Extraction Using Linear Prediction. *IEEE Trans Biomed Eng* 1989;36:1050-5.
5. Osowski S, Linh TH. ECG beat recognition using fuzzy hybrid neural network. *IEEE Trans Biomed Eng* 2001;48:1265-71.
6. Engin M. ECG beat classification using neuro-fuzzy network. *Pattern Recognit Lett* 2004;25:1715-22.
7. Jekova I, Bortolan G, Christov I. Assessment and comparison of different methods for heartbeat classification. *Med Eng Phys* 2008;30: 248-57.
8. Asl B, Setarehdan SK, Mohebbi M. Support vector machine-based arrhythmia classification using reduced features of heart rate variability signal. *Artif Intell Med* 2008;44:51-64.
9. Vaglio M, Couderc JP, McNitt S, Xia X, Moss AJ, Zareba W. A quantitative assessment of T-wave morphology in LQT1, LQT2, and healthy individuals based on Holter recording technology. *Heart Rhythm* 2008;5:11-8.
10. Couderc JP, McNitt S, Xia J, Zareba W, Moss AJ. Repolarization morphology in adult LQT2 carriers with borderline prolonged QTc interval. *Heart Rhythm* 2006;3:1460-6.
11. Boix M, Cantó B, Cuesta D, Micó P. Using the Wavelet Transform for T-wave alternans detection. *Math Comput Model* 2009;50:738-42.
12. Romero I, Grubb NR, Clegg GR, Robertson CE, Addison PS, Watson JN. T-wave alternans found in pre-ventricular tachyarrhythmias in CCU patients using a wavelet transform-based methodology. *IEEE Trans Biomed Eng* 2008;55:2658-65.
13. Jie Zhao, Jie Tian, Yan-Na Zhao, Ji-Kui Wang, Jian-Gong Xu, Fang-Zhou Xu. Detection of T-wave alternans based on the maximum of T waves. 3rd International Conference on Bioinformatics and Biomedical Engineering (ICBBE): Beijing; 2009. p. 1-4.
14. Ghaffari A, Homaeinezhad MR, Atarod M, Rahmani R. Detecting and quantifying T-wave alternans using the correlation method and comparison with the FFT-based method. *Conference on Computers in Cardiology: Bologna; 2008. p. 761-4.*
15. The MIT-BIH Normal Sinus Rhythm Database. Available from: <http://www.physionet.org/physiobank/database/nsrdb/> [Last accessed on 2010 Jun 01].
16. Laguna P, Mark R, Golberger A, Moody GB. A database for evaluation of algorithms for measurement of QT and other waveform intervals in the ECG. *Comp Card* 1997;24:673-6. Available from: <http://www.physionet.org/physiobank/database/qtdb/> [Last accessed on 2011 Sept 26].
17. T-Wave Alternans Challenge Database. Available from: <http://www.physionet.org/physiobank/database/twadb/>, [Last accessed on 2010 Jun 01].
18. Friesen GM, Jannett TC, Jadallah MA, Yates SL, Quint SR, Nagle HT. A comparison of the noise sensitivity of nine QRS detection algorithms. *IEEE Trans Biomed Eng* 1990;37:85-98.
19. RM Rangayyan. *Biomedical Signal Analysis: A Case Study Approach*. John Wiley & Sons, Inc., 2002.
20. Rangayyan RM. *Biomedical signal analysis: A case study approach*. New York: John Wiley and Sons, Inc.; 2002.

21. Chouhan VS, Mehta SS. Total removal of baseline drift from ECG signal, in Proceedings of International Conference on Computing: Theory and Applications: Kolkata; 2007. p. 512-5.
22. Zeraatkar E, Kermani S, Mehridehnavi AR, Aminzadeh A. Improving QRS detection for artifacts reduction. ICBME2010: 17th Iranian Conference on Biomedical Engineering: Isfahan; 2010. p. 1-4.
23. ChouhanVS, Mehta SS. Detection of QRS complexes in 12-lead ECG using adaptive quantized threshold. Int J Computer Sci Netw Secur 2008;8:155-63.
24. Krimi S, Ouni K, Ellouze N. T-Wave detection based on an adjusted wavelet transform modulus maxima. Int J Biol Sci 2006;1:128-32.
25. Li NQ, Wang ZS. T-Wave detection in electrocardiogram signal based on independent sub-band function. Intelligent Syst Appl 2009;2:1-3.
26. Tan KF, Chan KL, Choi K. Detection of the QRS-complex, P-wave, and T-wave in electrocardiogram. Proceedings of the First International Conference on Advances in Medical Signal Processing and Information Processing, IEE conference publication, No. 476. 2000. p. 41-7.
27. Daskalov IK, Christov Znd. Automatic detection of the electrocardiogram T-wave end. Med Biol Eng Comput 1999;37:348-53.
28. ChouhanVS, Mehta SS. Threshold-based Detection of P and T-wave in ECG using New Feature Signal. (IJCSNS) Int J Computer Sci Netw Secur 2008;8:144-53.
29. Haykin S. Neural Networks: A Comprehensive Foundation. New York: McMillan; 1994.
30. Mehridehnavi AR. Classification of the different cancerous animal tissues on the basis of their 1H NMR spectra using different types of Artificial Neural Networks. RPS Res Pharm Sci 2007;2:53-9.
31. Metz CE. Basic Principles of ROC Analysis. Semin Nucl Med 1978;8:283-98.
32. Goutas A, Ferdi Y, Herbeuval JP. Digital fractional order differentiation based algorithm for P and T-waves detection and delineation. ITBMRBM 2005;2:127-32.

How to cite this article: Zeraatkar E, Kermani S, Mehridehnavi A, Aminzadeh A, Zeraatkar E, Sanei H. Arrhythmia Detection based on morphological and time-frequency features of T-wave in electrocardiogram. J Med Sign Sens 2011;2:99-106

Source of Support: Nil, **Conflict of Interest:** None declared

BIOGRAPHIES



Elham Zeraatkar received her B.S. Degree in Electrical Engineering from Shariati Technical University (Iran) in 2004 and her M.Sc. degree in Biomedical Engineering from Departments of Physics and Biomedical Engineering, Isfahan University of Medical Sciences, Isfahan. Her interest is in biomedical signal processing, Fuzzy logic and Neural Network.



Saeed Kermani obtained his BS from the Department of Electrical Engineering of Isfahan University of Technology in Isfahan, Iran, 1987, and he received the MS in Bioelectric Engineering from Sharif University of Technology, in 1992 and his PhD in Bioelectric Engineering at AmirKabir University of Technology, Tehran, Iran, in 2008. He is Assistant Professor of Medical Engineering at the Department of Medical Physics and Medical Engineering in the School of Medicine of Isfahan University of Medical Sciences, Iran. His research interests are in biomedical signal and image processing techniques



Alireza Mehridehnavi was born in Isfahan province at 1961. He had educated in Electronic Engineering at Isfahan University of Technology at 1988. He had finished Master of Engineering in Measurement and Instrumentation at Indian Institute of Technology Roorkee (IIT Roorkee) in India at 1992. He has finished his PhD in Medical Engineering at Liverpool University in UK at 1996. He currently is an Associate

Professor of Medical Engineering at Medical Physics and Engineering Department in Medical School of Isfahan university of Medical Sciences.



A. Aminzadeh received his B.S. Degree in Electrical Engineering from Shiraz University (Iran) in 2000 and his M.Sc. degree in Control Engineering from Shiraz University in 2003. He has worked in a number of projects related to Real-Time Control, Multiple-Modeling and Heating-Plants. His current research interests include Classification of Biomedical Signals, Neural Networks, Electronic Control Unit of Internal Combustion Engines and Navigation Systems.



E. Zeraatkar received his B.S. Degree in Control Engineering from Shiraz University (Iran) in 2008 and his M.Sc. degree in Control Engineering from Shiraz University in 2012. His interest is in optimizing convergence in numerical methods such as Neural Networks. Recently he is focused on biomedical signal processing and classification methods for such signals.

Hamid Sanei obtained his MD in 1987, then graduated as a specialist in internal medicine and got his fellow in cardiovascular disease respectively in 1990 and 1996 Isfahan University of Medical Sciences, Iran. He is Associate Professor of cardiology and head of internal medicine department in the School of Medicine of Isfahan University of Medical Sciences, Iran. His research interests are cardiac signal, image and interventional cardiology.