

Application of Functional Near-Infrared Spectroscopy in Apraxia Studies in Alzheimer's Disease: A Proof of Concept Experiment

Apraxia refers to an impairment in performing consecutive movements and is among the early impairments in Alzheimer's disease (AD).^[1] In investigating brain areas involved in apraxia, functional magnetic resonance imaging (fMRI), and electroencephalography (EEG) are the mostly used neuroimaging techniques.^[2] This is while these are both highly sensitive to motion. An alternative to fMRI and EEG is functional near-infrared spectroscopy (fNIRS). fNIRS is less motion-sensitive which enables better data acquisition during motor tasks.^[3] In addition, fNIRS has a better temporal resolution compared to fMRI and offers a more precise localization of activity compared to EEG.^[4] However, despite these advantages, fNIRS has not yet been applied in the study of apraxia. Here, we present a proof of concept fNIRS experiment that offers some considerations for the design of an fNIRS study of apraxia in patients with neurodegenerative diseases.

In this experiment, we chose block design over an event-related task, because in this design, the stimuli are more predictable, making it easier for patients to maintain cognitive engagement.^[5] Furthermore, the hemodynamic responses are linearly summed when the brain is activated repeatedly as in block design, compensating for disrupted neurovascular coupling in neurodegenerative diseases.^[6] The task consists of two runs: (1) Observation, in which the subject should only observe the gestures and (2) imitation, in which the subject should imitate the gestures. Each run included three blocks of limb gestures and three blocks of oral gestures as these are the most common forms of apraxia in neurodegenerative diseases and have diagnostic value.^[7] A jittered 19.2s to 32s resting interval separated the blocks. Each block included five random gestures shown for 6s with a 1s interval in between [Figure 1]. The gestures were extracted from Dementia Apraxia Test.^[8] A 63-year-old AD patient and a 37-year-old healthy subject were recruited and informed consent was

obtained. A continuous-wave OxyMon fNIRS system (Artinis Medical Systems, Netherlands) with 28 active channels and a 10 Hz sampling rate was used. Measured wavelengths were 762 and 845 nm. Based on previous findings, the middle and superior parts of the temporal lobe, inferior and superior parts of the parietal lobe, and superior, middle, and inferior parts of the frontal lobe were selected as regions of interest.^[9-11] Location of optodes was determined using fNIRS Optodes' Location Decider^[12] and the most similar template was selected [Figure 2]. Raw data were processed using Homer3 in MATLAB 2021a (MathWorks, Natick, MA, USA).^[13] After the conversion of light intensity signals to an optical density (OD), a bandpass filter of 0.01–0.1 Hz was applied and targeted principle component analysis was performed.^[14] Changes in OD were then converted to concentration changes using modified Beer–Lambert Law.^[15] Concentration changes within a period of-2s before stimulus onset to 60s after stimulus onset (2s for baseline, 35s for five stimuli, and 23s for return to baseline) were averaged to obtain the hemodynamic response functions (HRF) during the task. Next, the HRF from channels within one region of interest (ROI) was averaged. Figures 3 and 4 demonstrate the HRF during the task. Overall, this experiment suggests that fNIRS can be used to study apraxia, especially in elderly patients with neurodegenerative diseases.

Statements

Statements section should be removed, because they are duplicated in Acknowledgement and Financial support sections.

Acknowledgment

The authors would like to acknowledge National Brain Mapping Laboratory, Tehran, Iran, for providing data acquisition service.

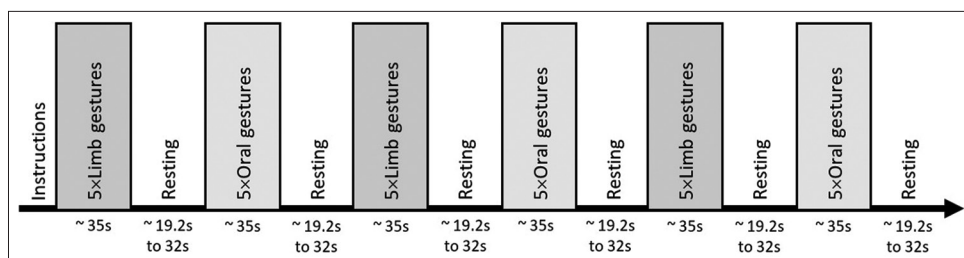


Figure 1: A single run of the task

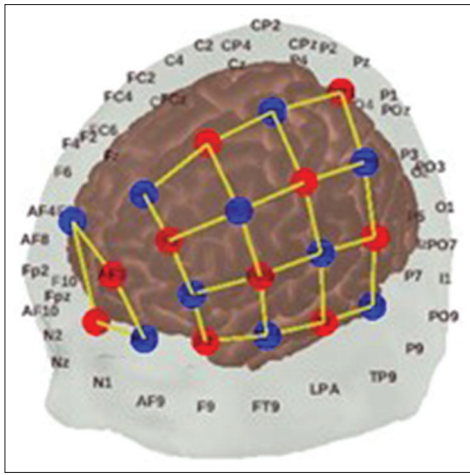


Figure 2: fNIRS optodes' template. fNIRS - Functional near-infrared spectroscopy

Declaration of patient consent

The authors certify that they have obtained all appropriate patient consent forms. In the form the patient(s) has/have given his/her/their consent for his/her/their images and other clinical information to be reported in the journal. The patients understand that their names and initials will not be published and due efforts will be made to conceal their identity, but anonymity cannot be guaranteed.

Financial support and sponsorship

This work was funded by Isfahan University of Medical Sciences.

Conflicts of interest

There are no conflicts of interest.

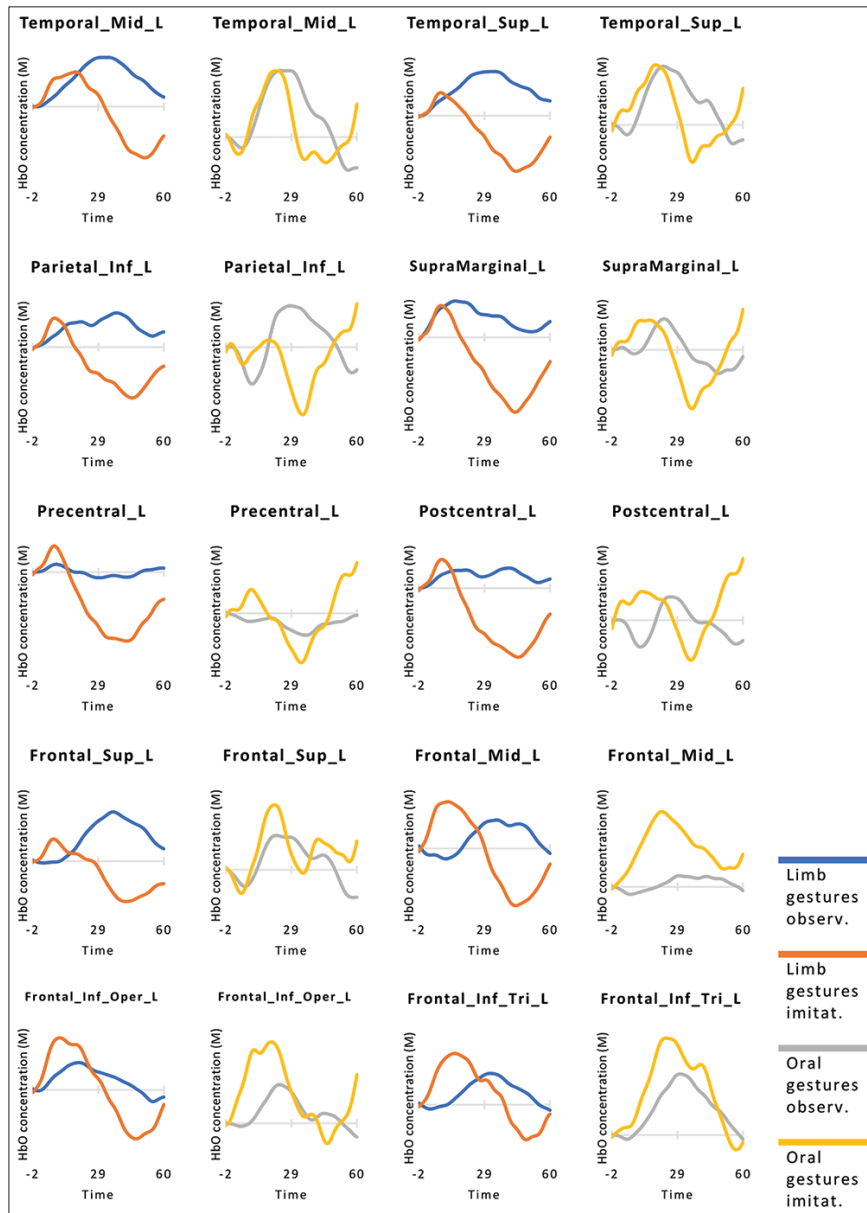


Figure 3: HRF during the task in an Alzheimer's patient. HRF - Hemodynamic response functions



Figure 4: HRF during the task in a healthy subject. HRF - Hemodynamic response functions

**Kiarash Azimzadeh, Majid Barekatin,
Farinaz Tabibian**

*Departments of Psychiatry, School of Medicine, Isfahan University of
Medical Sciences, Isfahan, Iran*

*Address for correspondence: Prof. Majid Barekatin,
Khorshid University Hospital, Isfahan City, Isfahan Province,
Isfahan, Iran.*

E-mail: barekatin@med.mui.ac.ir

Submitted: 29-May-2022 **Revised:** 10-Sep-2022

Accepted: 19-Sep-2022 **Published:** 31-Aug-2023

References

1. Johnen A, Tokaj A, Kirschner A, Wiendl H, Lueg G, Duning T, et al. Apraxia profile differentiates behavioural variant frontotemporal from Alzheimer's dementia in mild disease stages. *J Neurol Neurosurg Psychiatry* 2015;86:809-15.
2. Hallett M, de Haan W, Deco G, Dengler R, Di Iorio R, Gallea C, et al. Human brain connectivity: Clinical applications for clinical neurophysiology. *Clin Neurophysiol* 2020;131:1621-51.
3. Herold F, Wiegel P, Scholkmann F, Thiers A, Hamacher D, Schega L. Functional near-infrared spectroscopy in movement science: A systematic review on cortical activity in postural and

walking tasks. *Neurophotonics* 2017;4:041403.

4. Quaresima V, Ferrari M. Functional Near-Infrared Spectroscopy (fNIRS) for assessing cerebral cortex function during human behavior in natural/social situations: A concise review. *Organ Res Methods* 2019;22:46-68.
5. D'Esposito M, Zarahn E, Aguirre GK. Event-related functional MRI: Implications for cognitive psychology. *Psychol Bull* 1999;125:155-64.
6. Shan ZY, Wright MJ, Thompson PM, McMahon KL, Blokland GG, de Zubicaray GI, *et al.* Modeling of the hemodynamic responses in block design fMRI studies. *J Cereb Blood Flow Metab* 2014;34:316-24.
7. Johnen A, Reul S, Wiendl H, Meuth SG, Duning T. Apraxia profiles-A single cognitive marker to discriminate all variants of frontotemporal lobar degeneration and Alzheimer's disease. *Alzheimers Dement (Amst)* 2018;10:363-71.
8. Johnen A, Frommeyer J, Modes F, Wiendl H, Duning T, Lohmann H. Dementia apraxia test (DATE): A brief tool to differentiate behavioral variant frontotemporal dementia from Alzheimer's dementia based on apraxia profiles. *J Alzheimers Dis* 2016;49:593-605.
9. Yliranta A, Jehkonen M. Limb and face apraxias in frontotemporal dementia: A systematic scoping review. *Cortex* 2020;129:529-47.
10. Rosenzopf, H., Wiesen, D., Basilakos, A., Yourganov, G., Bonilha, L., Rorden, C., Fridriksson, J., Karnath, H. O., & Sperber, C. (2022). Mapping the human praxis network: an investigation of white matter disconnection in limb apraxia of gesture production. *Brain communications*, 4(1), fcac004. <https://doi.org/10.1093/braincomms/fcac004>.
11. Pizzamiglio G, Zhang Z, Kolasinski J, Riddoch JM, Passingham RE, Mantini D, *et al.* A role for the action observation network in apraxia after stroke. *Front Hum Neurosci* 2019;13:422.
12. Zimeo Morais GA, Balardin JB, Sato JR. fNIRS Optodes' location decider (fOLD): A toolbox for probe arrangement guided by brain regions-of-interest. *Sci Rep* 2018;8:3341.
13. Huppert TJ, Diamond SG, Franceschini MA, Boas DA. HomER: A review of time-series analysis methods for near-infrared spectroscopy of the brain. *Appl Opt* 2009;48:D280-98.
14. Yücel MA, Selb J, Cooper RJ, Boas DA. Targeted principle component analysis: A new motion artifact correction approach for near-infrared spectroscopy. *J Innov Opt Health Sci* 2014;7:1350066.
15. Kocsis L, Herman P, Eke A. The modified Beer-Lambert law revisited. *Phys Med Biol* 2006;51:N91-8.

This is an open access journal, and articles are distributed under the terms of the Creative Commons Attribution-NonCommercial-ShareAlike 4.0 License, which allows others to remix, tweak, and build upon the work non-commercially, as long as appropriate credit is given and the new creations are licensed under the identical terms.

Access this article online	
Quick Response Code:	Website: www.jmssjournal.net
	DOI: 10.4103/jmss.jmss_40_22

How to cite this article: Azimzadeh K, Barekatin M, Tabibian F. Application of functional near-infrared spectroscopy in apraxia studies in Alzheimer's disease: A proof of concept experiment. *J Med Sign Sens* 2023;13:319-22.

Downloaded from <http://journals.lww.com/jmss> by BhDMf5ePHKav1zEoum1tQIN4a+kJLhEZgbsIHo4XMI0hCywCXT1AW nYQplI0hID333D00dRy7T7Sf4c3V4OA/vPDDa8K2+Ya6H515KE= on 10/24/2023